


J&M MSP800 UV-VIS Microspectrophotometer with Leica DM4000



Spectra measured with this system:

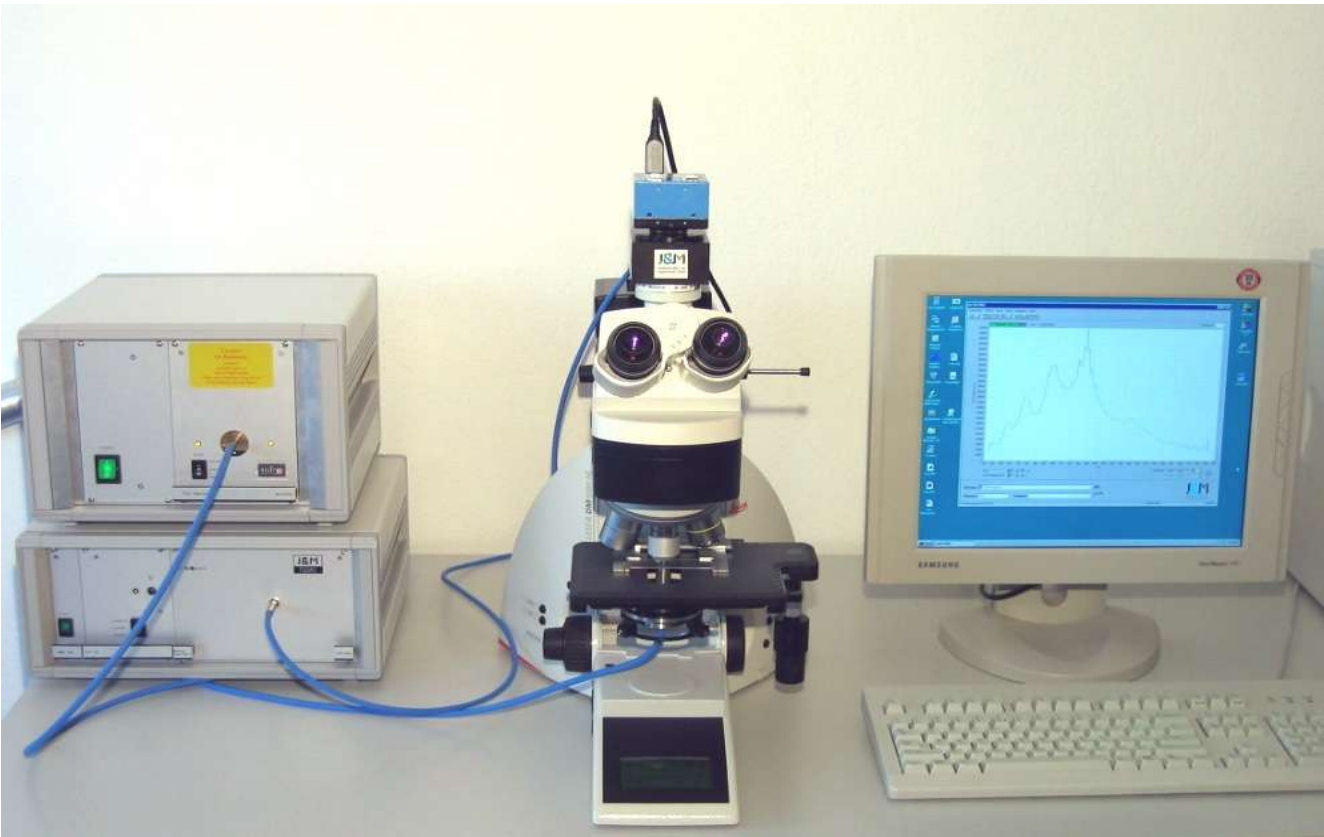